

# AMPLATZER™ AMULET™ LAA OCCLUDER DEMONSTRATES SAFETY AND EFFECTIVENESS THROUGH 3 YEARS



STROKES IN WATCHMAN‡ PATIENTS WERE MORE FREQUENTLY PRECEDED BY DEVICE-RELATED FACTORS (DEVICE-RELATED THROMBUS, DRT; OR PERI-DEVICE LEAK, PDL) THAN STROKES IN AMULET PATIENTS

Ischemic Stroke Patient Details (6 Months – 3 Years)*	Amulet (n=29)	Watchman‡ (n=29)
Device factors**		
Device-related thrombus	1	2
Peridevice leak (≥3mm)	3	15
OAC usage at time of stroke	0	3



\* Aspirin only recommended for both groups after 6 months  
 \*\* Device factors had to occur prior to the stroke occurrence to be counted  
 OAC - Oral Anticoagulation

BOTH CARDIOVASCULAR DEATH AND ALL-CAUSE DEATH TRENDED LOWER AT 3 YEARS WITH AMULET THAN WATCHMAN‡<sup>†</sup>

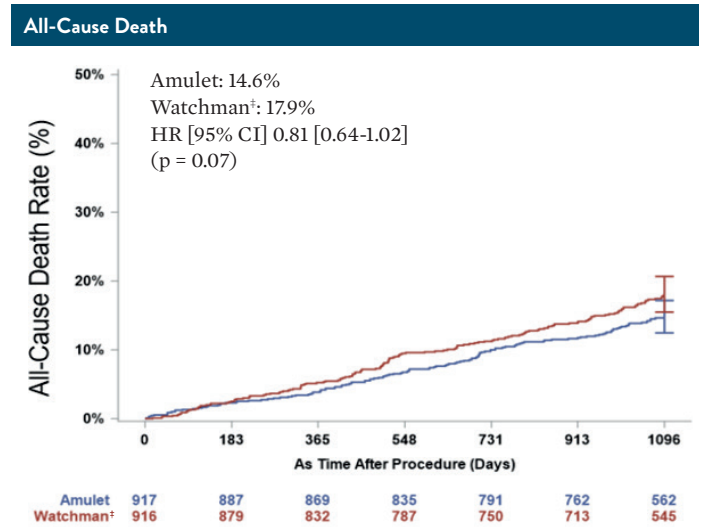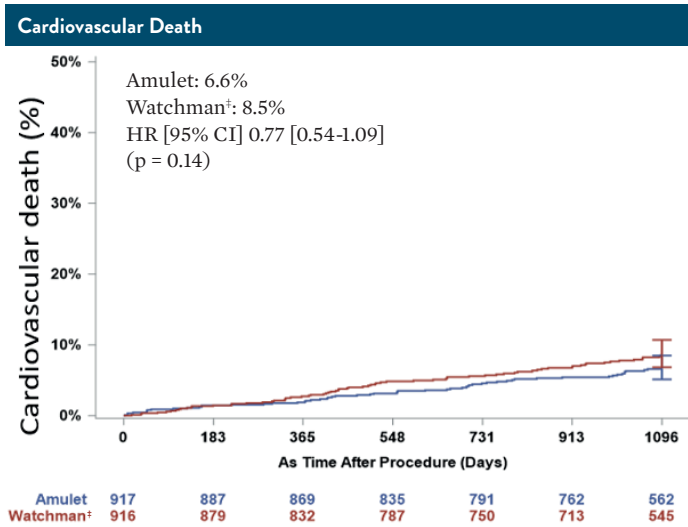

1. Descriptive analysis of non-powered endpoints in a population with differential long-term follow-up at 3 years

Lakkireddy et al. 3-Year Outcomes from the Amplatzer™ Amulet™ Left Atrial Appendage Occluder Randomized Controlled Trial (Amulet IDE), presented at TCT 2022.

**CAUTION:** This product is intended for use by or under the direction of a physician. Prior to use, reference the Instructions for Use, inside the product carton (when available) or at [efu.abbottvascular.com](http://efu.abbottvascular.com) or at [medical.abbott/manuals](http://medical.abbott/manuals) for more detailed information on Indications, Contraindications, Warnings, Precautions and Adverse Events.

Information contained herein for DISTRIBUTION outside of the U.S. ONLY. Always check the regulatory status of the device in your region. Illustrations are artist's representations only and should not be considered as engineering drawings or photographs. Photo(s) on file at Abbott.

**Abbott**  
 3200 Lakeside Dr., Santa Clara, CA. 95054 USA  
[www.structuralheart.abbott](http://www.structuralheart.abbott)

™ Indicates a trademark of the Abbott group of companies.  
 ‡ Indicates a third-party trademark, which is property of its respective owner.  
 © 2022 Abbott. All rights reserved. MAT-2211648 v2.0 | Item approved for OUS use only.

